

DreamStation 2

Auto CPAP Advanced

Introducing
DreamStation 2
Auto CPAP Advanced
Success. By design.



Introducing DreamStation 2 Auto CPAP Advanced



22% smaller

than a leading competitor

29% smaller than
DreamStation

16% lighter

than a leading competitor

32.5% lighter than DreamStation
(with power supply included)

Device components



Water tank
with lid



Reusable
pollen filter



Ultrafine
pollen filter


Evolving to a new way of doing business

The business of treating patients for obstructive sleep apnea (OSA) is more complex than ever. The need to minimize personal contact and increase connectivity has led to the heightened importance of home delivery.

There is a clear need for simplified, low-touch solutions that help you get patients started on sleep therapy quickly, safely and comfortably while continuing to grow your business.

Philips DreamStation 2 Auto CPAP Advanced provides a streamlined user experience for enhanced operational efficiencies in setup times and training, patient initiation and patient management.

The OSA Journey

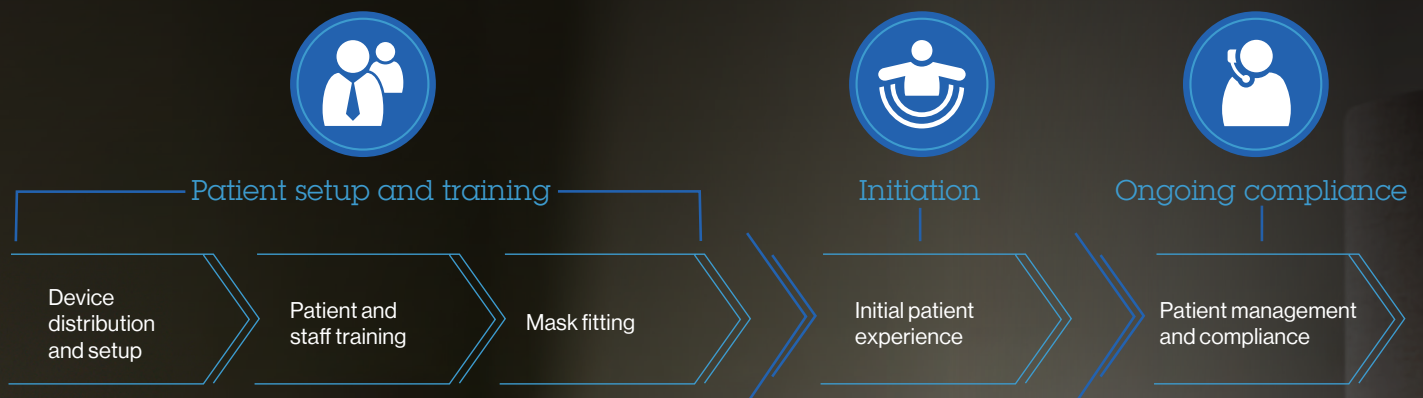

Philips DreamStation 2 Auto CPAP Advanced Success. By design.

Simplified.
Intuitive.
Connected.



DreamStation 2 Auto CPAP Advanced is designed to help you and your patients succeed...together.




Patient setup and training

Efficient setup: Flexibility in the setup process allows you to choose what is best for your business.

1. Out-of-the-box, no-touch setup¹
 - Accept data-driven defaults
 - Personalize remotely with Care Orchestrator
2. Streamlined, low-touch, first-ever guided setup on the device

Simplified training: The CPAP features intuitive navigation of comfort features and settings, along with easy handling of the device.

Precision mask fitting: Philips Respironics Mask Selector uses no-touch scanning technology for the right mask fit from the start.²



RTs set up **DreamStation 2 Auto CPAP Advanced** 28.7% faster than DreamStation on first try.³



Initiation

Three easy-to-access comfort settings: Patients can make live adjustments of Ramp Plus, humidification and heated tube temperature while therapy is running.

- Ramp Plus allows patients to set a comfortable starting pressure for falling asleep, which may also help reduce callbacks and adjustments to minimum pressure prescriptions.

Micro-flexible 12mm heated tube: Philips smallest-diameter tubing is designed to be comfortable while taking up less space than traditional tubing.

Smart auto and advanced algorithms: Proprietary algorithms automatically adjust pressure to provide personalized therapy and treat AHIs at lower pressures.⁴




Ongoing compliance

Enhanced connectivity: Integrated cell modem with simplified Bluetooth pairing enables remote setup and easy access to data for both your care team and your patients.

- On-demand prescription changes
- Remote troubleshooting through Performance Check

Philips Care Orchestrator: Drive collaboration among your team with patient insights delivered straight to smartphones, tablets or PCs.

- Adherence Profiler enables you to get notifications if a patient is at risk of noncompliance in a 90-day period.



DreamMapper app keeps patients engaged with easy access to coaching to drive ongoing compliance.

Patients struggling with adherence to sleep therapy have a 283% higher success rate.⁵

Ordering information

DreamStation 2 Auto CPAP Advanced part numbers	
Description (Package Label)	Part number
DreamStation 2 Auto CPAP Advanced + Humidifier with cell/BT	DSX520H11C
DreamStation 2 Auto CPAP Advanced + Humidifier/Heated Tube with cell/BT	DSX520T11C

DreamStation 2 Auto CPAP Advanced	
Description (Package Label)	Part number
DS2 Humidifier Water Tank No Lid, RP	1146072
DS2 Humidifier Lid only, RP	1146073
DS2 Water Tank with Lid	1142832
DS2 Inlet/Outlet Seal, RP	1142836
DS2 Reusable Pollen Filter, RP – 1 pack	1142687
DS2 Disposable Ultra-Fine Filter, RP – 1 pack	1142828
DS2 Disposable Ultra-Fine Filter, RP – 2 pack	1142829
DS2 Disposable Ultra-Fine Filter, RP – 6 pack	1142831
3150 BLE Wrist Ox	1144877
Soft Reusable Finger Sensor, WristOx, SM	1147077
Soft Reusable Finger Sensor, WristOx, M	1147178
Soft Reusable Finger Sensor, WristOx, L	1147179
PC USB Interface Cable, WristOx 3150 BLE	1147180
DS2 Carrying Case	1142834
DreamStation 2 Roll Stand	1145156

DreamStation 2 Auto CPAP and DreamStation 2 Auto CPAP Advanced	
Description (Package Label)	Part number
15mm Heated Tube	HT15
RP - 15mm Standard Tube - DreamStation	PR15
DreamStation Micro-Flexible 12mm Tube RP	PR12
HT12 Heated Tube	HT12
22mm Performance Tube	1032907
DreamStation 12mm Tube Device Adapter w/OIS	1147466
Philips RI SD Card – 1 pack	1145085
Philips RI SD Cards – 10 pack	1063859
EN: Shielded DC Cord - DreamStation	1120746
EN: Shielded DC Cord System - DreamStation	1120747
Philips 80W CPAP Power Supply	1144267
Power Cord w/C7 END-USA/CAN	1005894
DC Battery Adapter Cable	532209
PAP Lithium Ion Battery Kit	1124009
Lithium Ion Battery, PAP Device Cable	1121736
Lithium Ion Battery Case	1126947
Bacteria Filter	342077
Pressure Valve	302418
O ₂ Enrichment Attachment	312710

References:

1. Assumes acceptance of smart, default settings. Alternatively, you can set up prescriptions entirely via CO with no device touch.
2. Data analysis after 90 days of use. 2019 Philips sponsored patient preference trial (n=310). Patient scanned using the Mask Selector (n=153) vs. Traditional fitting methods (n=157).
3. Philips randomized usability trial. Ease-of-Set Up and Time-to-Set Up of Continuous Positive Airway Pressure (CPAP) Devices; evaluating the user interface with 27 respiratory therapists that typically set up Philips DreamStation and ResMed AirSense 10 CPAP devices. 2020.
4. Hertegonne KB, Rombaut B, Houtmeyers P, Van Maele G, Pevernagie DA. Titration efficacy of two auto-adjustable continuous positive airway pressure devices using different flow limitation-based algorithms. *Respiration*. 2008;75(1):48-54. doi: 10.1159/000103515. Epub 2007 Jun 1. PMID: 17541262. Nolan GM, Ryan S, O'Connor TM, McNicholas WT. Comparison of three auto-adjusting positive pressure devices in patients with sleep apnoea. *Eur Respir J*. 2006 Jul;28(1):159-64. doi: 10.1183/09031936.06.00127205. Epub 2006 Mar 29. PMID: 16571610. Nieves Navarro Soriano, Mikel Azpiazu Blocona, Javier Carrillo Hernández-Rubio, Raquel Cobos Campos, Ainhoa Alvarez Ruiz de Larrinaga, Bereniç Murià Diaz David Diez Fuente, Carlos Javier Egea Santaolalla. The Effective Pressure of the CPAP Titration Depends on the APAP Device Used. Poster at SEPAR Convention (Spain). May 2018. Javier Carrillo Hernandez-Rubio, Mikel Azpiazu Blocona, David Diez Fuente, Nieves Berlen Navarro Soriano, Laura Cancelo Diaz, Lourdes Guerra Martin, Raquel Cobos Campos, Carlos Javier Egea Santaolalla. Validity of the CPAP Automatic Titration in our Sleep Unit. Poster at SEPAR Convention (Spain). May 2018.
5. 46% of DreamMapper patients went on to achieve adequate adherence within 90 days versus 12% for the Standard Care group, a relative increase of 283.33%. In a retrospective review conducted by Philips Respironics of the EncoreAnywhere database (white paper) of struggling patients (n=24,176).

For more information please contact us at:

Air Liquide Healthcare, Stratus House, Unit 1 IDA College Park, Blanchardstown Road North, Blanchardstown, Dublin 15, D15 PEC4.

Tel: +353 (0)1 809 1800 Freephone: 1800 24 02 02 (ROI only) 0800 328 5875 (NI only)

Fax: +353 (0)1 829 3966 Email: healthie@airliquide.ie Website: www.airliquidehealthcare.ie